

USER GUIDE AND SPECIFICATIONS

NI WSN-3202

NI Wireless Sensor Network 4-Channel, 16-Bit Analog Input Node

This user guide describes how to use the NI WSN-3202 analog input node and lists its specifications. Figure 1 shows the NI WSN system components.

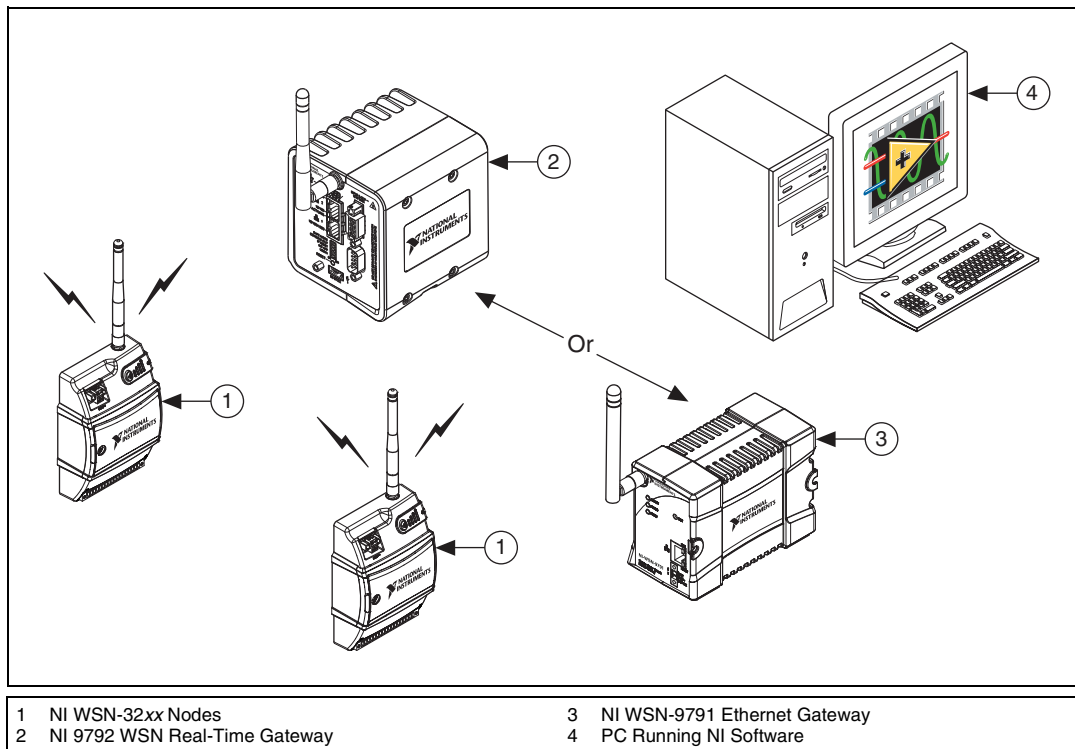


Figure 1. NI WSN System Components

The NI WSN-3202 is a four-channel, low-power, wireless voltage input device that works with other NI WSN-32xx nodes and gateways to form a wireless sensor network. The NI WSN system consists of one or more NI WSN gateways, up to 36 NI WSN-32xx nodes per gateway, and multiple PCs or Programmable Automation Controllers (PACs) to receive and analyze the distributed sensor data. For more information about PACs, visit ni.com.

When you connect the NI WSN gateway, you can use a separate host PC running Windows, or a PAC running NI LabVIEW Real-Time, to display measurement results, status information, and to change the NI WSN gateway and NI WSN-3202 device settings. Figure 2 shows the NI WSN-3202 device block diagram.

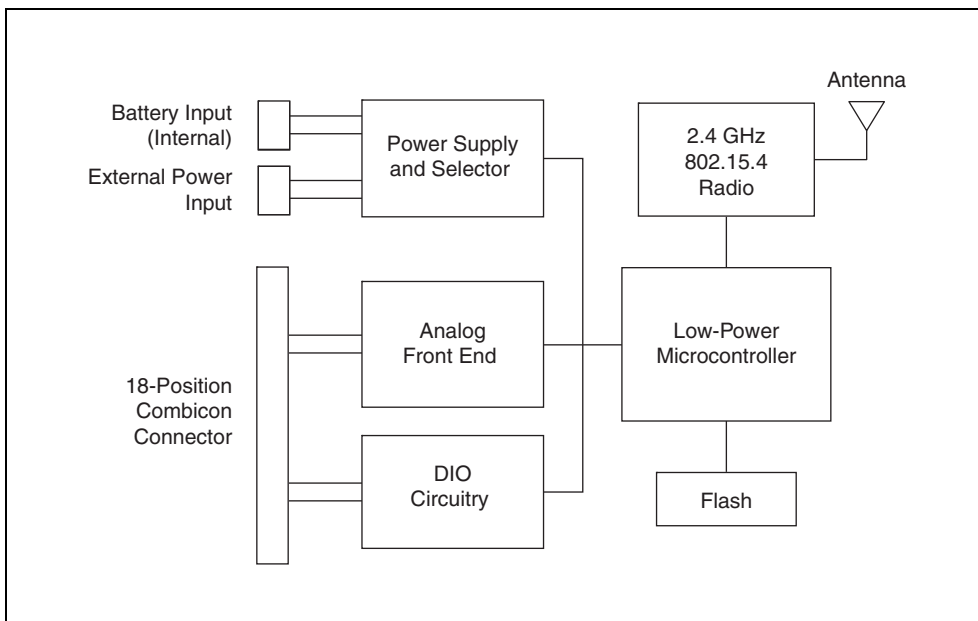


Figure 2. NI WSN-3202 Block Diagram

Dimensions

Figure 3 shows the NI WSN-3202 device dimensions.

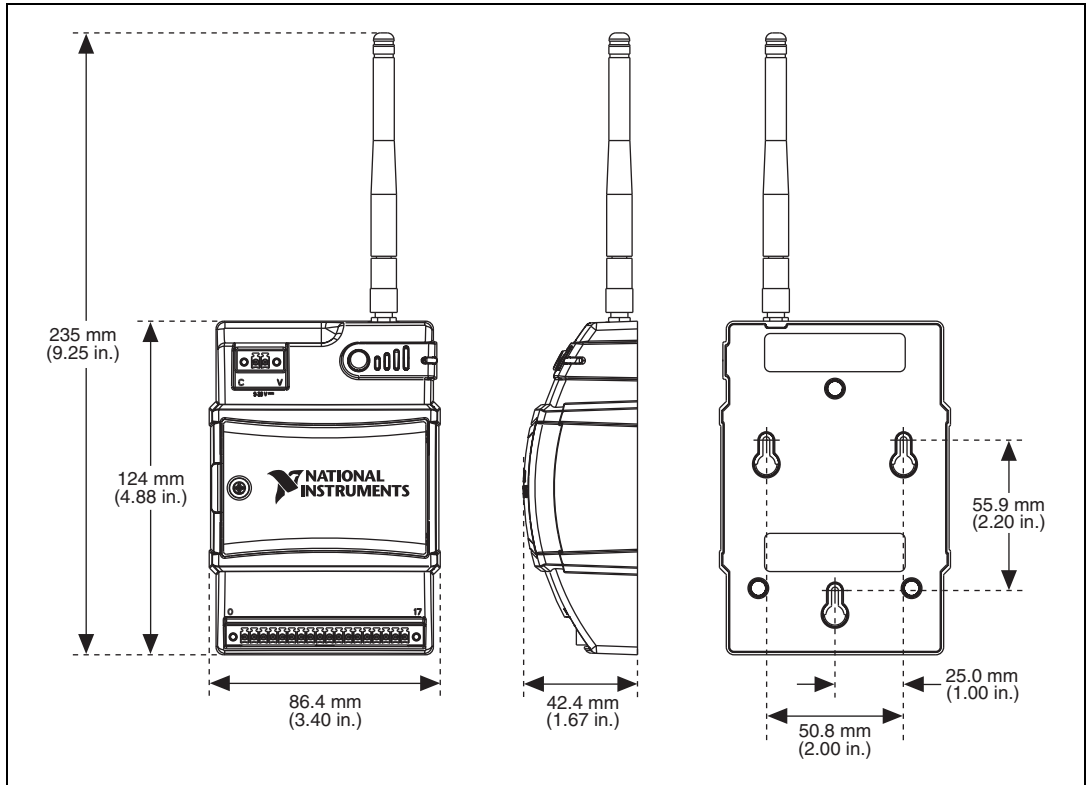


Figure 3. NI WSN-3202 Device Dimensions

Safety Guidelines

Operate the NI WSN-3202 device only as described in this user guide.



Hot Surface This icon denotes that the component may be hot. Touching this component may result in bodily injury.

NI WSN Safety Information

The following section contains important safety information that you *must* follow when installing and using NI WSN products.



Caution Do not operate the NI WSN product in a manner not specified in the user manual or operating instructions. Product misuse can result in a hazard. You can compromise the safety protection built into the product if the product is damaged in any way. If the product is damaged, return it to National Instruments for repair.



Caution Do not substitute parts or modify the NI WSN product. Use the product only with the devices, accessories, and cables specified in the installation instructions.



Caution Do *not* operate NI WSN products in an explosive atmosphere or where there may be flammable gases or fumes.



Caution If you need to clean a NI WSN product, wipe it with a dry towel. The product *must* be completely dry and free from contaminants before you return it to service.



Caution Operate the product indoors only at or below Pollution Degree 2. Pollution is foreign matter in a solid, liquid, or gaseous state that can reduce dielectric strength or surface resistivity.



Caution You *must* insulate signal connections for the maximum voltage for which the NI WSN product is rated. Do *not* exceed the maximum ratings for the product. Do *not* install wiring while the product is live with electrical signals. Do *not* remove or add connector blocks when power is connected to the NI WSN system. Avoid contact between your body and the connector block signal wiring when hot-swapping devices.



Caution To comply with safety regulations, use only recommended batteries with this product. Refer to the [Battery Power](#) section for the recommended battery types.

Safety Guidelines for Hazardous Locations

The NI WSN-3202 is suitable for use in Class I, Division 2, Groups A, B, C, D, T4 hazardous locations; Class I, Zone 2, AEx nC IIC T4 and Ex nL IIC T4 hazardous locations; and nonhazardous locations only. Follow these guidelines if you are installing the NI WSN-3202 in a potentially explosive environment. Not following these guidelines may result in serious injury or death.



Caution Observe the battery manufacturers' operating temperature ratings listed in the [Battery operating temperature range](#) specification section.



Caution Do not disconnect the power supply wires and connectors from the device unless power has been switched off.



Caution Do not install or remove the device unless power has been switched off.



Caution Substitution of components may impair suitability for Class I, Division 2.



Caution For Zone 2 applications, install the WSN system in an enclosure rated to at least IP 54 as defined by IEC 60529 and EN 60529.

Special Conditions for Hazardous Locations Use in Europe

The NI WSN-3202 has been evaluated as Ex nA nL IIC T4 equipment under DEMKO Certificate No. 07 ATEX 0626664X. Each device is marked II 3G and is suitable for use in Zone 2 hazardous locations, in ambient temperatures of $-40\text{ }^{\circ}\text{C} \leq T_a \leq 70\text{ }^{\circ}\text{C}$.

Electromagnetic Compatibility Guidelines

This product was tested and complies with the regulatory requirements and limits for electromagnetic compatibility (EMC) as stated in the product specifications. These requirements and limits are designed to provide reasonable protection against harmful interference when the product is operated in its intended operational electromagnetic environment.

This product is intended for use in industrial locations. There is no guarantee that harmful interference will not occur in a particular installation, when the product is connected to a test object, or if the product is used in residential areas. To minimize the potential for the product to cause interference to radio and television reception or to experience unacceptable performance degradation, install and use this product in strict accordance with the instructions in the product documentation.

Furthermore, any changes or modifications to the product not expressly approved by National Instruments could void your authority to operate it under your local regulatory rules.

The following statements contain important EMC information needed before installing and using this product:



Caution To ensure the specified EMC performance, product installation requires either special considerations or user-installed, add-on devices. See the product installation instructions for further information.



Caution To ensure the specified EMC performance, operate this product only with shielded cables and accessories.



Caution This product may become more sensitive to electromagnetic disturbances in the operational environment when test leads are attached or when connected to a test object.

Related Documentation

Check ni.com/manuals for the most recent documentation. For a complete list of documentation related to the NI WSN system, refer to ni.com/info and enter `rdwsnrd`.

In addition to this guide, the following documents may be useful when configuring your NI WSN system:

- *NI Wireless Sensor Network Getting Started Guide*
- *NI WSN-9791 Ethernet Gateway User Guide and Specifications*
- *NI 9792 WSN Real-Time Gateway User Guide and Specifications*
- *Configuring WSN in MAX*, available from **Start»All Programs»National Instruments»NI-WSN**
- *LabVIEW Help for WSN Devices*, available in LabVIEW from **Help»LV Help»WSN Devices Help**
- *NI-WSN Readme*, available on the software installation disc included with your gateway

Training Courses

If you need more help getting started developing an application with NI products, NI offers training courses. To enroll in a course or obtain a detailed course outline, refer to ni.com/training.

Technical Support on the Web

For additional support, refer to ni.com/support or zone.ni.com.

Software Overview



Note Refer to the *NI WSN Readme*, available on the software installation disc included with your device, for NI software application version support.

The NI-WSN software includes NI Measurement & Automation Explorer (MAX) as well as server and driver software for easy integration into application software packages. These software components manage the low-level communications and hardware configurations, simplifying programmatic access to I/O channels. The NI-WSN software is on the software installation disc included with your NI WSN gateway device. The NI-WSN software is supported by Windows 7/Vista/XP and contains the following components:

- NI MAX
- NI-WSN

You can download a current version of NI-WSN software from ni.com/support. Using your Web browser, go to ni.com/support and select **Drivers and Updates»Distributed I/O»Wireless Sensor Networks**, and then select the latest version of NI-WSN software. If you are using other software, refer to the installation instructions that accompany your software.

What You Need to Get Started

To set up and use NI LabVIEW with the NI WSN-3202 device, you need the following:

- NI WSN gateway
- NI WSN 32xx devices with a 9–30 V power supply or four AA 1.5 V alkaline batteries for each node. Refer to the [Battery Power](#) section for recommended batteries.
- Mounting hardware (DIN rail, panel-mount, or rack mount accessory)
- Ethernet cable/connection
- 1/8 in. flathead and number 2 Phillips screwdrivers
- NI-WSN software version 1.0 or later
- Host PC running Windows 7/Vista/XP
- NI LabVIEW 8.6.1 (32-bit) or later
- **(NI 9792 WSN Real-Time Gateway Only)** NI LabVIEW 2009 SP1 (32-bit) Real-Time Module or later
- Related hardware and software documentation

Unpack the Device and Install the Antenna

Remove the device from the package and inspect the device. Contact NI if the device appears damaged. Do *not* install a damaged device.



Caution The device is static sensitive. Always properly ground yourself and the equipment when handling or connecting to the device.

To attach the antenna, align the antenna with the mount and screw it on as shown in Figure 4.



Caution The antenna must be attached to the NI WSN devices in order for the NI WSN devices to function correctly.

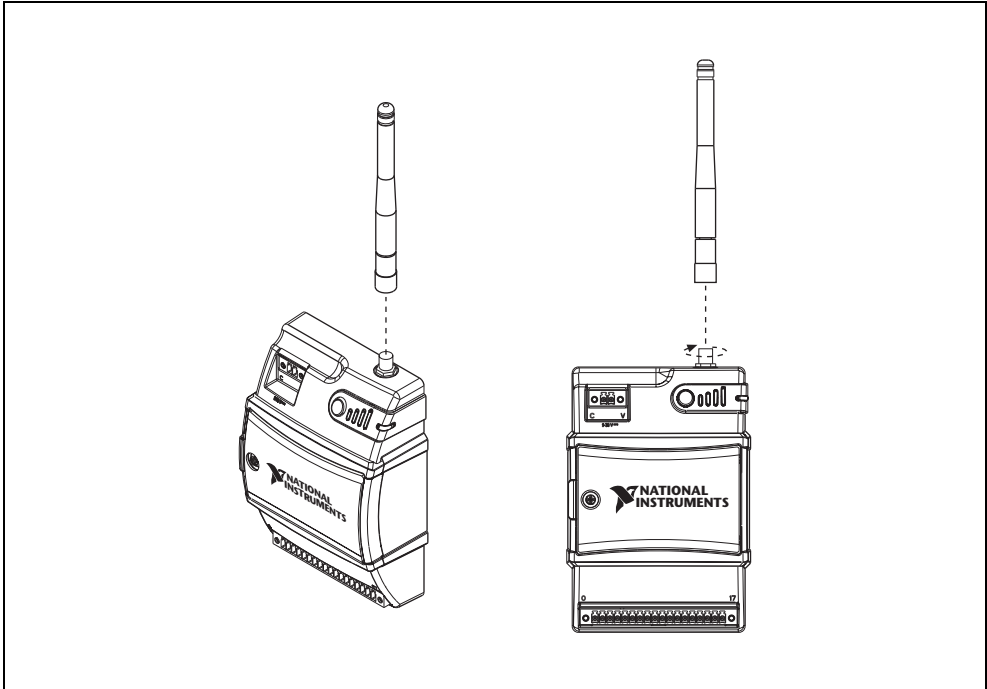


Figure 4. Attach the Antenna to the Device

Mounting the NI WSN-3202 Device

You can mount the NI WSN-3202 on a panel or on a 35 mm DIN rail. For kit accessory ordering information, refer to the NI WSN product page accessory section at ni.com. Before using any of these mounting methods, remove and save the serial number sticker located on the back of the NI WSN-3202 device for future use when configuring your device in software. For the NI WSN-3202 device dimensions, refer to Figure 3.



Caution Your installation *must* allow 50.8 mm (2 in.) of clearance in front of devices for common connector cabling, such as the 18-terminal detachable screw terminal connector.

Attaching the NI WSN-3282 DIN Rail (Optional)

You can mount the NI WSN-3202 on a standard 35 mm DIN rail using a NI WSN-3282 DIN rail clip, NI part number 781074-01. Complete the following steps to mount the NI WSN-3202 on a DIN rail:



Caution Power off the device before mounting it to the DIN rail.



Note Use thread-forming screws to permanently affix the DIN rail clip to the device. Unscrewing and reinstalling the thread-forming screws will produce a compromised connection between the DIN rail clip and the device.

1. Fasten the DIN rail clip to the NI WSN-3202 using a number 2 Phillips screwdriver and the four 8-32 \times 5/16 in. thread-forming screws that shipped with the DIN rail clip. Figure 5 shows how to fasten the DIN rail clip to the NI WSN-3202.



Caution Do *not* use screws longer than 5/16 in. to fasten the DIN rail clip to the NI WSN-3202.

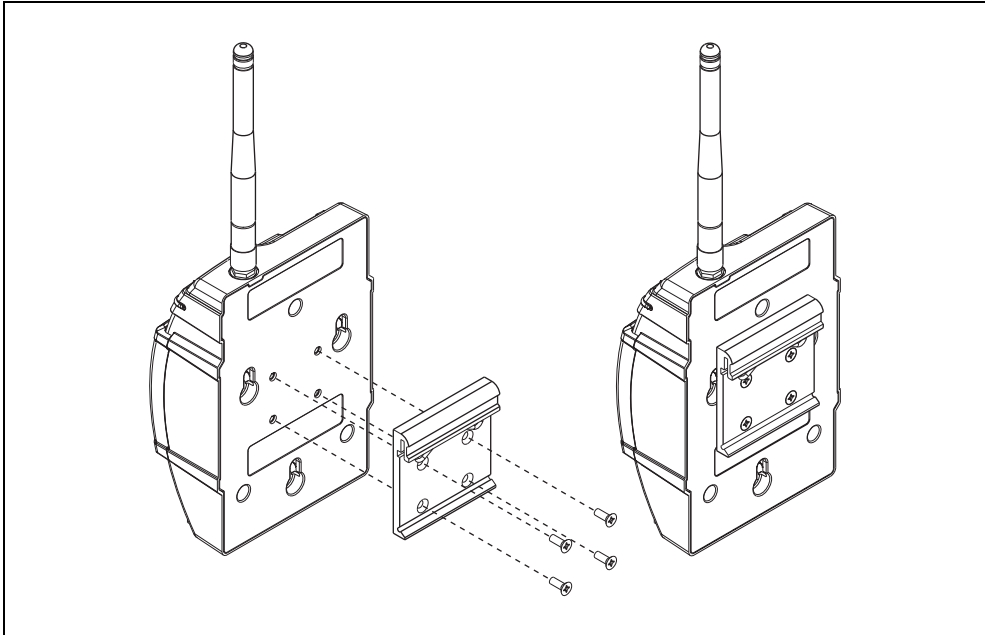


Figure 5. NI WSN-3202 Device DIN Rail Installation

2. Insert one edge of the DIN rail into the deeper opening of the DIN rail clip, as shown in Figure 6.

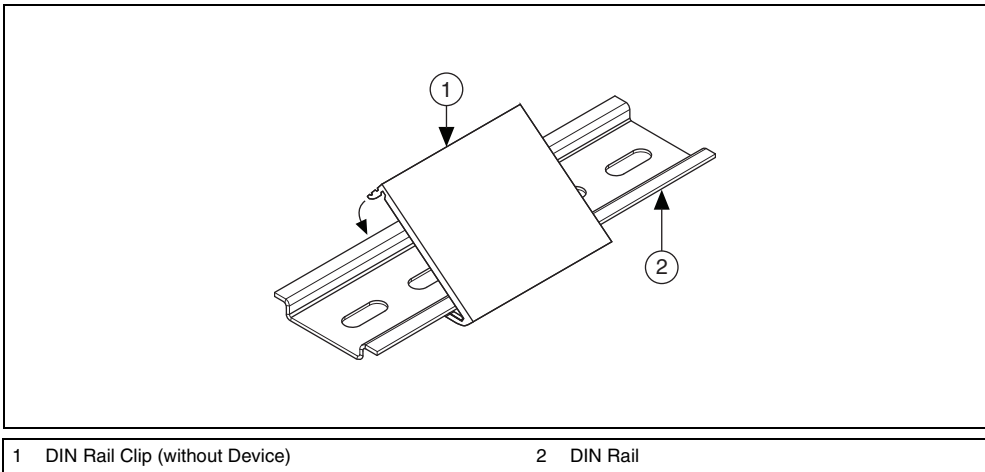


Figure 6. DIN Rail Clip Installation

3. Press down firmly on the NI WSN-3202 to compress the spring until the clip locks into place on the DIN rail.

Using a Panel Mount Accessory

The NI WSN-3280/3281 panel mount accessories, part numbers 780999-01 and 781073-01, each include a retention clip and knob and integrated strain relief for power and I/O wires. You can use the NI WSN-3280 panel mount accessory to attach the NI WSN-3202 device to a panel or other flat surface. The NI WSN-3281 panel mount accessory also includes a magnetic mount for attaching the NI WSN-3202 device to metallic surfaces. Figure 7 shows the NI WSN-3202 panel mounting dimensions.

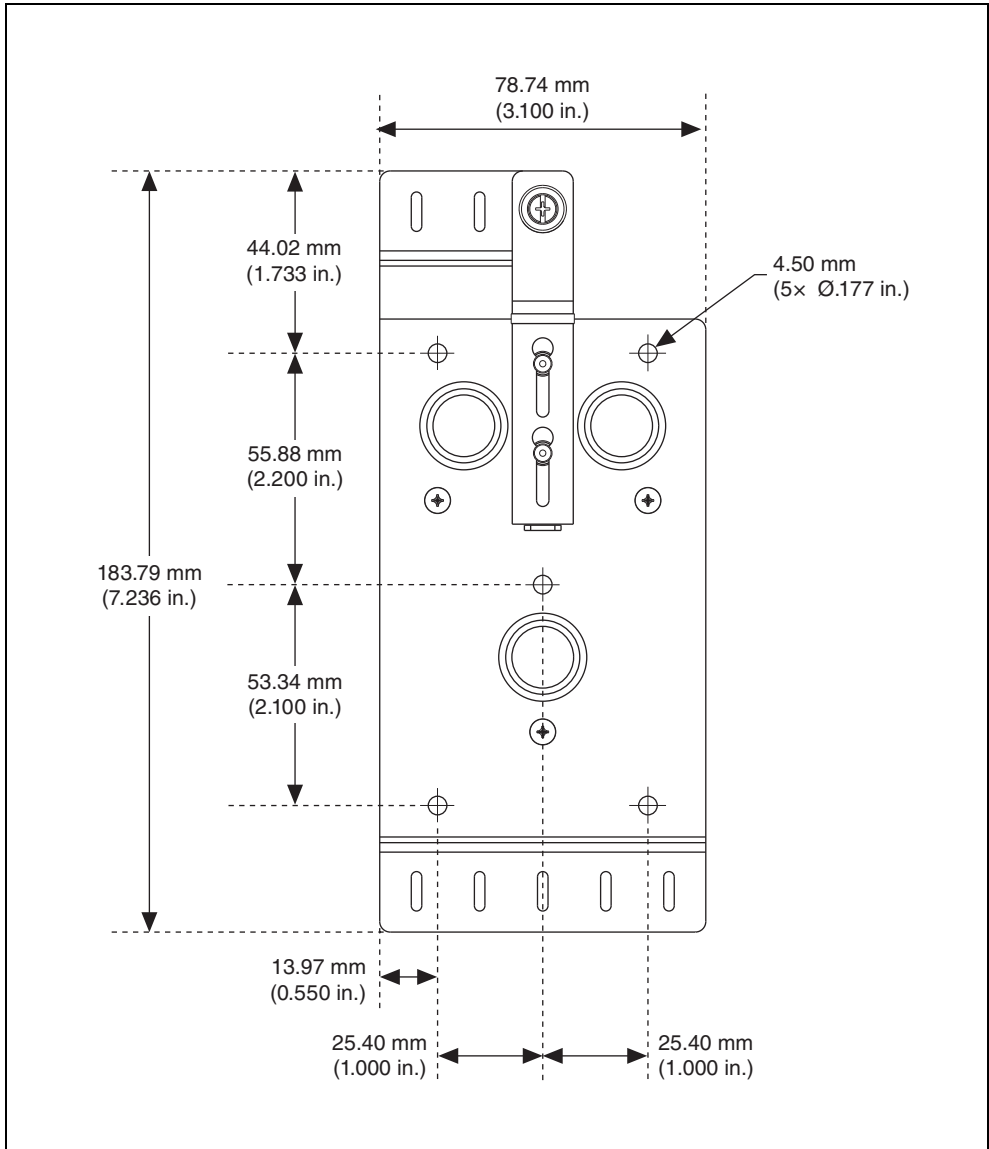


Figure 7. NI WSN-3202 Device Panel Mount Dimensions

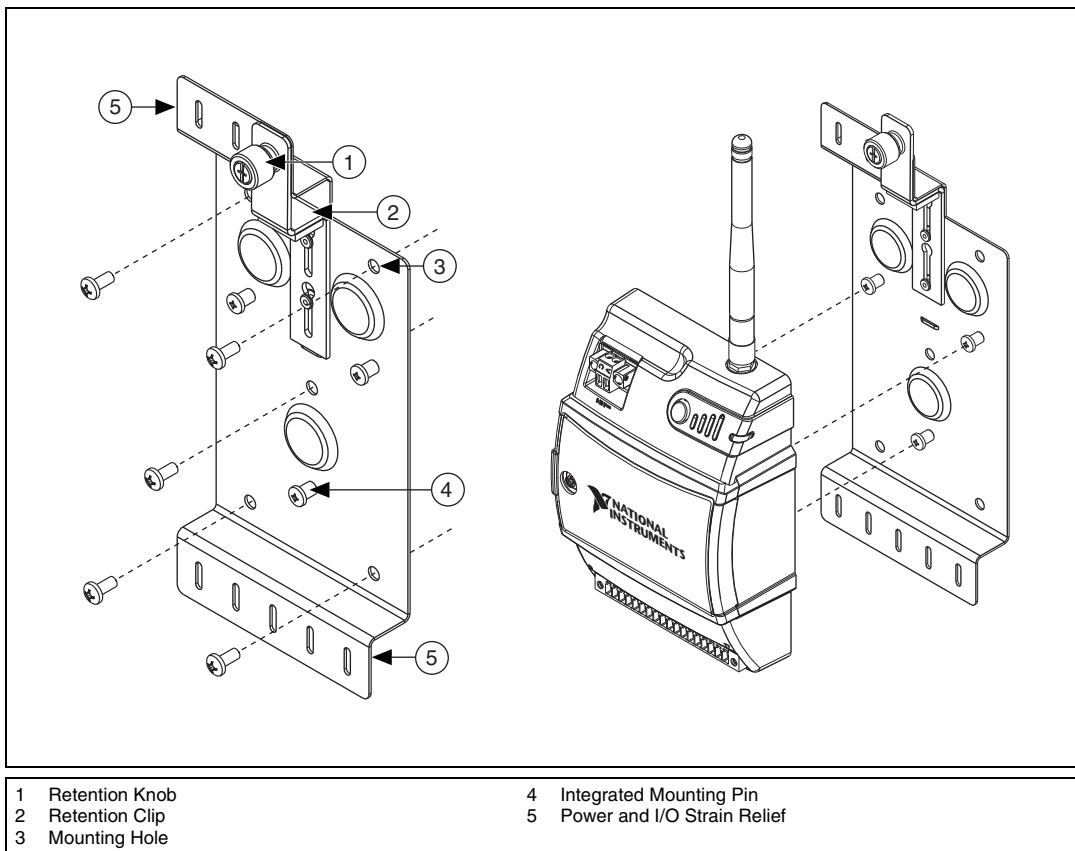


Figure 8. Panel Mount Accessory

Refer to Figure 8 while completing the following steps to mount the NI WSN-3202 on a panel:

1. **(NI WSN-3280)** Bolt or screw the panel mount accessory to a panel using five 8-32 or M4 screws.
(NI WSN-3281) Attach the panel mount accessory using the integrated magnet.
2. Slide the NI WSN-3202 device into the panel mount accessory as shown in Figure 8.

3. Slide the retention clip down and tighten the panel mount knob to secure the NI WSN-3202 device as shown in Figure 9.

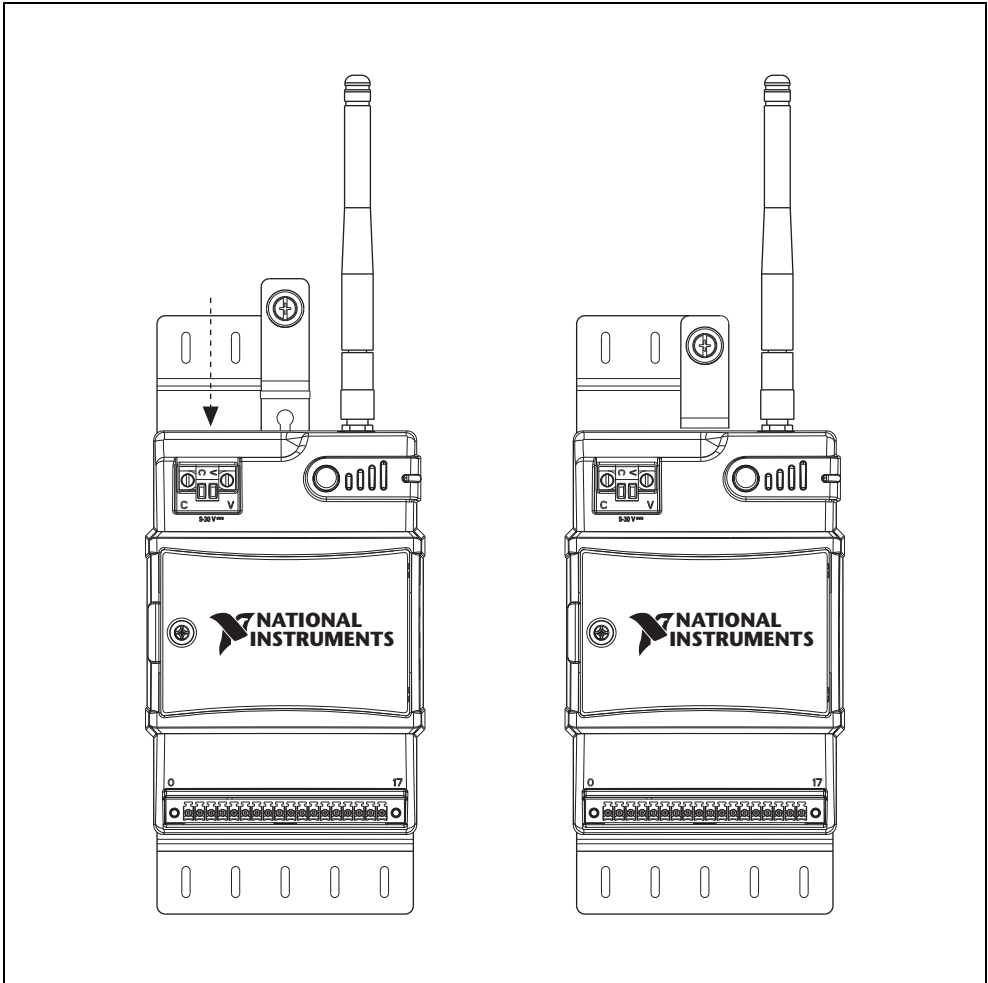


Figure 9. Slide Retention Clip Down and Tighten Panel Mount Knob

4. (Optional) Secure any I/O signal or power supply cabling to the panel mount accessory using a zip-tie and the integrated strain relief slots.

Using the Integrated Panel Mount Slots

You can also mount the NI WSN-3202 to a panel using the integrated panel mount slots as shown in Figure 10.

1. Attach three number 8 or M4 pan head screws in the mounting panel, leaving 0.1 in. space under the head of each screw. Refer to Figure 3 for the correct hole pattern and dimensions.
2. Slide the NI WSN-3202 device onto the panel.



Note In this configuration, the NI WSN-3202 is held in place only by the weight of the device and the screw attachment friction. Use the DIN rail clip or panel mount accessories in high vibration environments.

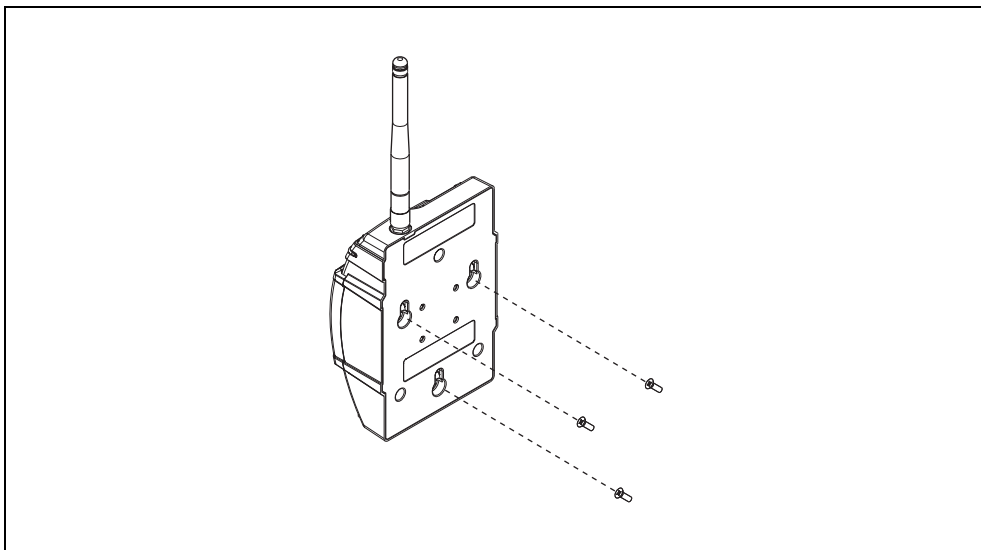


Figure 10. Integrated Panel Mount Slots



Caution Disconnect power before removing the device from the panel.

Setting Up the NI WSN-3202 Device

The following sections discuss setting up the NI WSN-3202 for use.

Installing the Software

You must be an Administrator to install NI software and devices on your computer. Before connecting the hardware, install the following software in the following order:

1. NI LabVIEW, available at ni.com/support.
2. NI-WSN and NI MAX, which are included on the software installation disc included with your NI WSN gateway and are also available for download at ni.com/support.



Note After installation of NI-WSN, the *NI Wireless Sensor Network Getting Started Guide* is available from **Start»All Programs»National Instruments»NI-WSN**.

Powering the NI WSN-3202 Device

The NI WSN-3202 device can be powered on by either an external power supply or four AA alkaline batteries. Refer to the [Specifications](#) section for details about the input power and battery requirements.

If both battery and external power are connected, the NI WSN-3202 functions from the external power input. The device is designed to provide battery backup in the event of loss of external power and will automatically switch to battery power when external power is lost.

Installing Batteries

To install batteries in the NI WSN-3202 device, complete the following steps:

1. Loosen the battery compartment retention screw and remove the compartment cover, as shown in Figure 11.

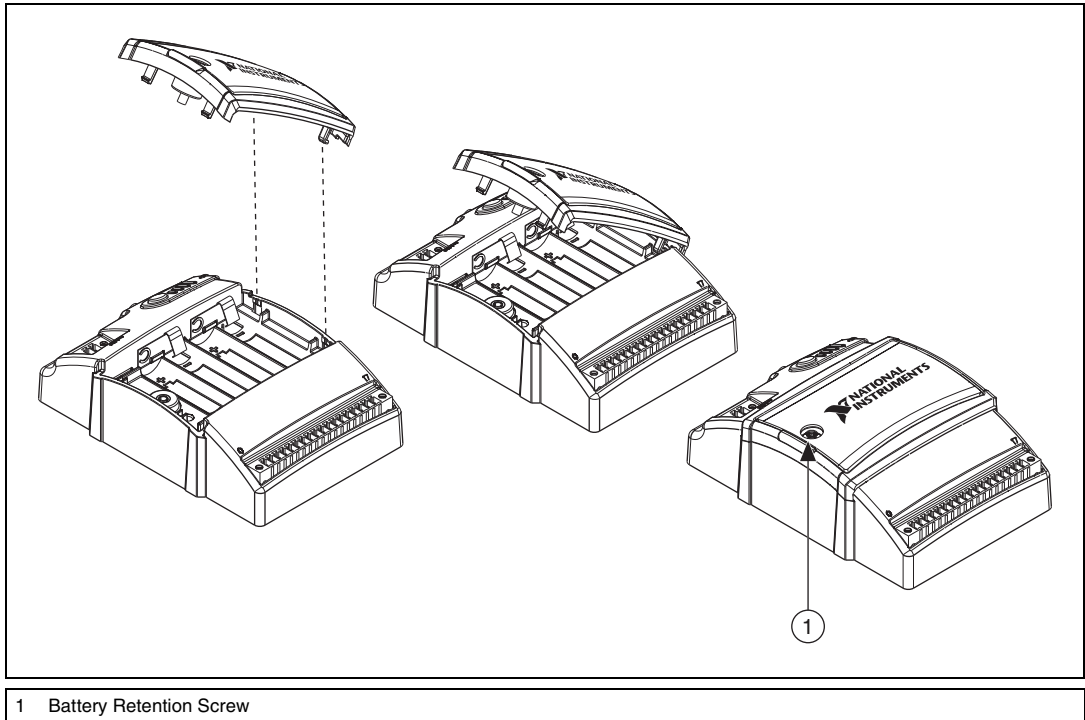


Figure 11. NI WSN-3202 Battery Compartment



Caution Using the incorrect battery type causes an explosion risk. Do *not* use rechargeable batteries. Refer to the [Battery Replacement and Disposal](#) section for information about how to dispose of used batteries.



Note When using the NI WSN-3202 device on battery power, you should configure the device as an end node so that it sleeps most of the time. Running a device configured in router mode from battery power greatly reduces the battery life. The device ships from the factory configured as an end node. For more information about how to switch the node from end mode to router mode, refer to *Configuring WSN in MAX*, available from **Start»All Programs»National Instruments»NI-WSN**.

2. Install four AA alkaline batteries in to the device, making sure to install them with the correct polarity. Figure 13 shows the battery polarity markings inside the device battery compartment.
3. Reinstall the battery compartment cover and tighten the retention screw.

Connecting External Power to the NI WSN-3202 Device

To connect an external power supply to the NI WSN-3202, complete the following steps:

1. Remove the 2-position mini-combicon plug from the device, loosening the retaining screws if necessary.

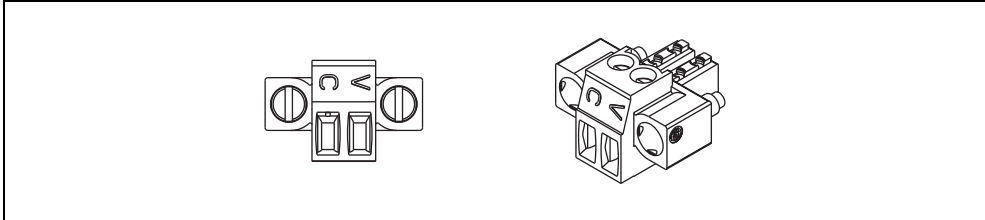


Figure 12. 2-Position Mini-Combicon Plug

2. Connect the external power supply positive lead to the V terminal.
3. Connect the negative (common) lead to the C terminal.
4. Reinstall the 2-position mini-combicon plug in the device and tighten the retaining screws.



Caution You must use a UL Listed ITE power supply marked LPS with the NI WSN-3202. The power supply must also meet any safety and compliance requirements for the country of use.

Device Interface

Figure 13 shows the NI WSN-3202 device interface.

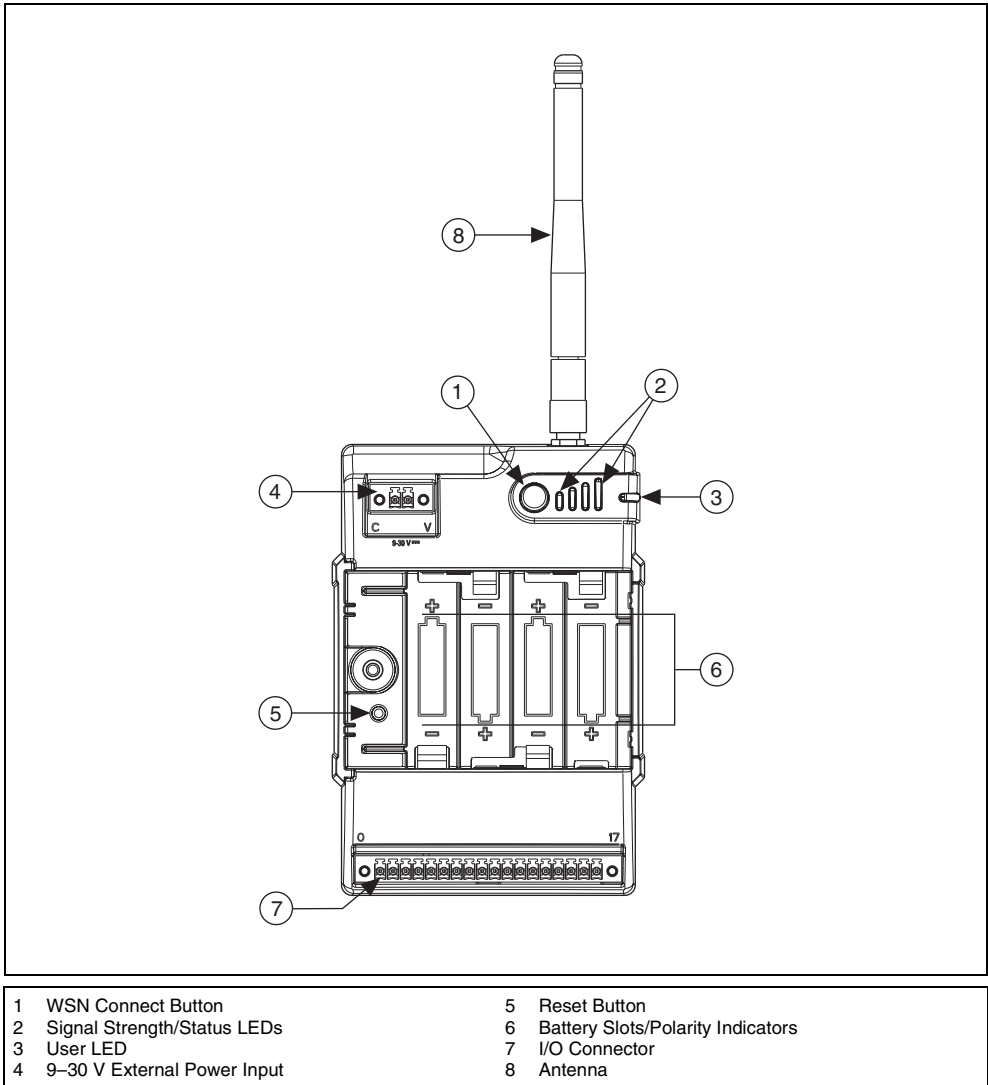










Figure 13. NI WSN-3202 Node Interface

Signal Strength/Status LED Indicators

The NI WSN-3202 has four signal strength/status LED indicators, which flash twice before displaying signal strength information. Table 1 shows the status and signal strength LED patterns.

Table 1. Signal Strength and Status LED State/Node Status

LED Indication Mode	LED State	LED Pattern	Device Status
Signal Strength—LEDs 1–4 blink twice and then display the signal strength for three seconds	LED 1–4 OFF		Low Signal
	LED 1 ON, LED 2–4 OFF		Poor
	LED 1–2 ON, LED 3–4 OFF		Fair
	LED 1–3 ON, LED 4 OFF		Good
	LED 1–4 ON		Excellent
Status Indication	Each LED 1–4 blinking in succession		Searching for network
	LED 1, 4 and 2, 3 alternate blinking		Updating firmware
	LED 1–4 continuously blinking		Error. Reboot device. If problem persists, reset device to factory default settings. Go to ni.com/support for additional troubleshooting steps.

WSN Connect Button



Note Refer to your NI WSN gateway documentation for detailed instructions about how to connect a NI WSN-3202 to the NI WSN gateway.

The NI WSN-3202 is equipped with a WSN connect button as shown in Figure 13. The button controls network connection and the LEDs, which display connection status.

Pressing the WSN connect button results in the device responses shown in Table 2.

Table 2. WSN Connect State/Device Status

Current Device State	Duration of Button Press	Result
Initial power on, not connected	Any duration	Node turns on and searches for an available network.
Connected to a NI WSN-9791	<5 seconds	Node blinks all four signal strength LEDs twice, and then displays the signal strength as shown in Table 1.
	≥5 seconds	Node leaves current network and searches for a new network.

Reset Button

The NI WSN-3202 is equipped with a reset button as shown in Figure 13.

Pressing the reset button results in the following device responses:

- When pressed for fewer than five seconds, the device reboots with the current configuration.
- When pressed for five seconds or more, the device reboots into Factory Default Mode, which returns the device user configuration to the factory-set defaults.

Analog Input Circuitry

Terminals 0–7 on the 18-position screw terminal connector are analog input. Each channel has an AI terminal to which you can connect a voltage signal and an AI GND terminal which is internally connected to the device analog ground reference.

The input signals are filtered, conditioned, and then sampled by a single 16-bit ADC. Figure 14 shows the NI WSN-3202 input circuitry.

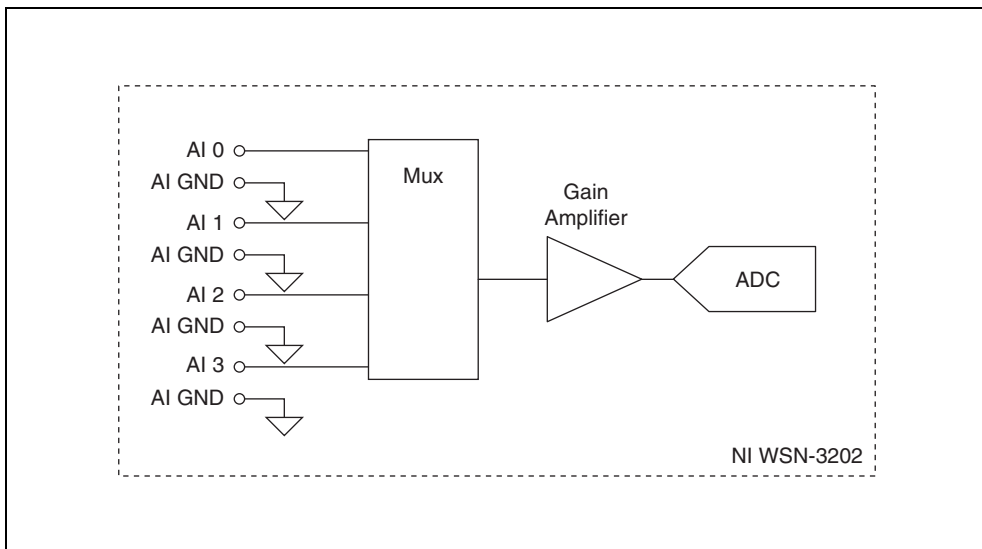


Figure 14. NI WSN-3202 Input Circuitry

Connecting Analog Inputs to the NI WSN-3202

You can connect single-ended voltage signals to the NI WSN-3202. For single-ended connections, connect the voltage signal positive lead to AI x . Connect the ground signal to AI GND. Each AI GND terminal is internally connected to the device analog ground. Figure 15 shows a single-ended voltage signal connected to the NI WSN-3202.

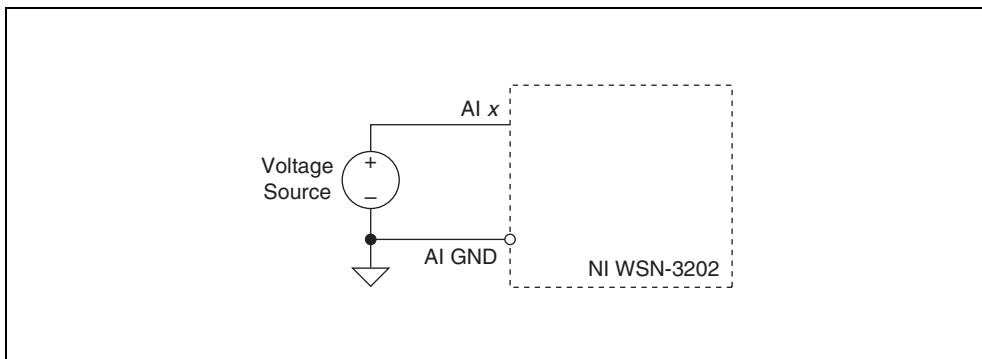


Figure 15. Connecting a Single-Ended Voltage Signal

Minimizing Measurement Errors

The NI WSN-3202 analog ground is internally connected to the digital ground. Avoid introducing common-mode errors in the analog measurement by using separate ground wires for the analog and digital signals, as shown in Figure 16.

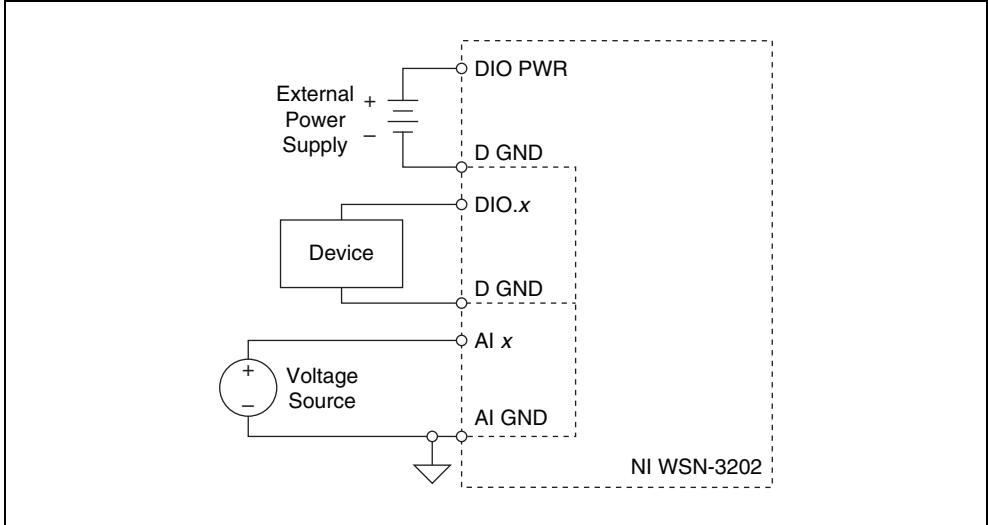


Figure 16. Recommended Method of Separating Analog and Digital Ground Wires

If the analog and digital signals must share a common ground wire, as shown in Figure 17, use a larger wire gauge to reduce this error as much as possible. The screw terminal can accept up to 14 AWG wire.

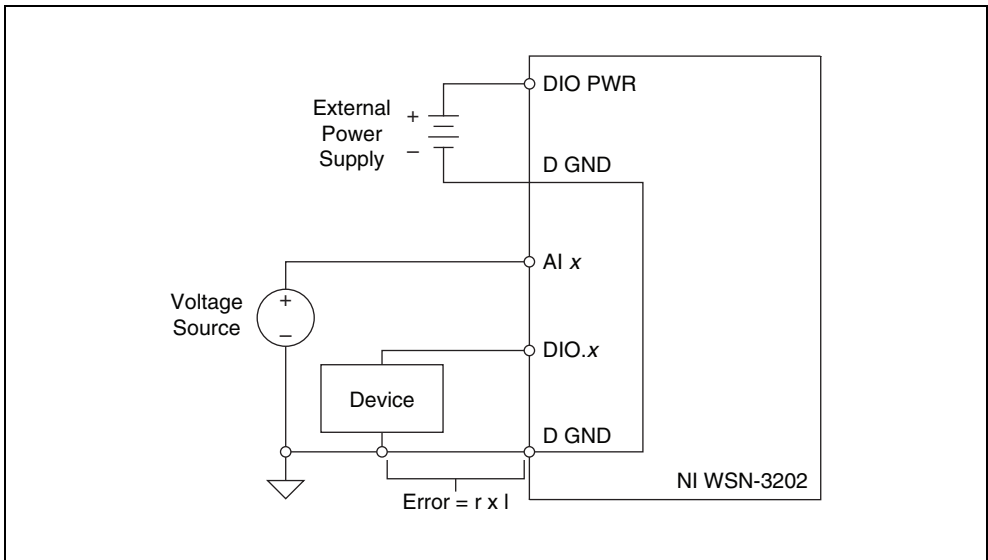


Figure 17. Using a Single Ground Wire Introduce Common-Mode Errors

To minimize measurement error use a thick wire for the ground connection.

Powering an External Sensor

The NI WSN-3202 device can provide up to 20 mA at 12 V to external sensors through its sensor power (SEN PWR) terminal. You can configure this sensor power output using NI-WSN software to turn on a sensor up to 250 ms prior to the start of an acquisition. Figure 18 shows the sensor power circuit connected to a device.

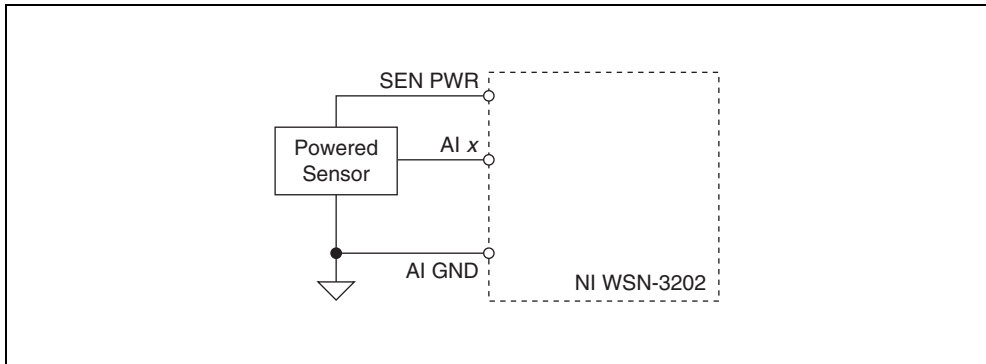


Figure 18. Powering an External Sensor with the NI WSN-3202

Make sure the device you are connecting is compatible with the NI WSN-3202 sensor power circuit voltage and current ranges. Refer to the [Specifications](#) section for more information.

Controlling Digital Inputs and Outputs

The NI WSN-3202 device has four bi-directional digital I/O channels, and each channel supports four operational modes: Drive High Only, Drive Low Only, Drive High and Low, and Tristate. Use the **Node Properties** dialog box in the LabVIEW Project Explorer window to change DIO settings.

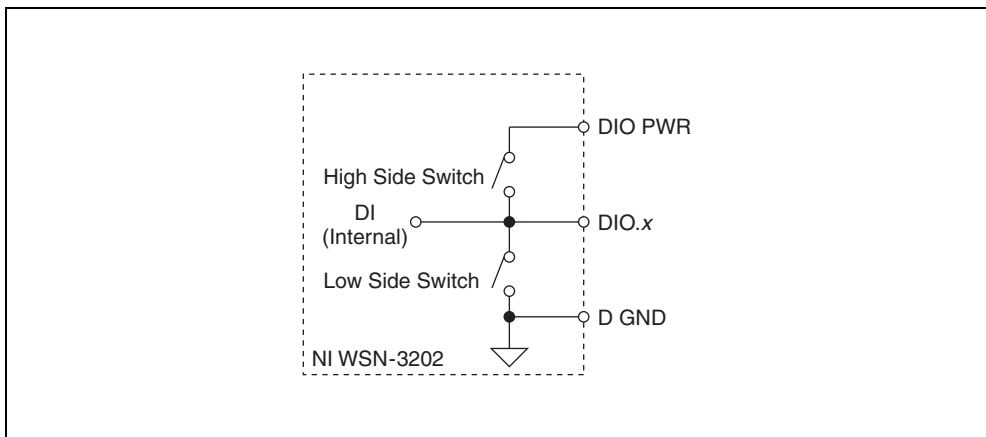


Figure 19. Simplified Circuit Diagram of One DIO Channel

Terminals 9–17 are the DIO section on the 18-position screw terminal connector. Each DIO channel has a signal terminal (DIO.x) and a ground terminal (D GND). There is also a terminal for the positive terminal of DIO Power (DIO PWR), which is only required when one of the DIO channels is configured for sourcing output. There is an internal Digital Input terminal which reads the digital output current state or the value of DIO.x when configured for Tristate mode. The NI-WSN software controls the different modes of operation by turning on and off the high side and low side switches.

You can connect a variety of industrial devices such as solenoids, relays, and indicators to the NI WSN-3202 device. Refer to the [Specifications](#) section to ensure compatibility. The Drive High Only and the Drive High and Low modes require an external power supply connected to the DIO PWR terminal.

The following sections discuss how to configure the NI WSN-3202 device for different types of input and output and how to connect external devices to the NI WSN-3202 DIO terminals.

Connecting Sourcing Digital Outputs

You must connect an external power supply to the NI WSN-3202 to source digital outputs. This power supply provides the current for the devices you connect to the NI WSN-3202. Connect the power supply positive lead to DIO PWR terminal and the power supply negative lead to one of the D GND pins. The DIO PWR terminal on the NI WSN-3202 is internally connected to each digital channel. You can connect only one external voltage supply to the device. Refer to the [Specifications](#) section for information about the power supply voltage range.



Note You must use 2-wire ferrules to create a secure connection when connecting more than one wire to a single terminal on the NI WSN-3202.

You can connect sourcing digital outputs to the NI WSN-3202 in either Drive High Only Mode or Drive High and Low Mode. In either mode, connect the device to DIO.x and connect the device common to the D GND terminal closest to that DIO.x terminal.

Drive High Only Mode

In Drive High Only Mode, the DIO.x terminal is driven to the voltage supplied to DIO PWR when you turn on the channel. Writing a digital value of 1 turns on the channel, and 0 turns off the channel. The channel is high impedance (refer to the [Digital Input \(Tristate Mode\)](#) specification) when the channel is turned off (0). Use this mode for devices that require high side drive or a sourcing output.

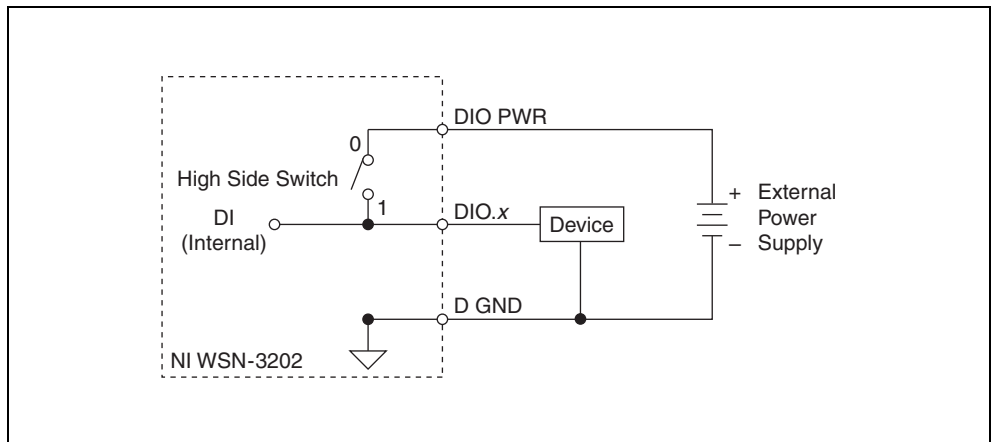


Figure 20. Connecting a Device to the NI WSN-3202 in Drive High Only Mode

Drive High and Low Mode

In Drive High and Low mode, the DIO.x terminal is driven to the voltage supplied to DIO PWR when you turn on the channel, and is driven to D GND when you turn off the channel. Writing a digital value of 1 turns on the channel, and 0 turns off the channel.

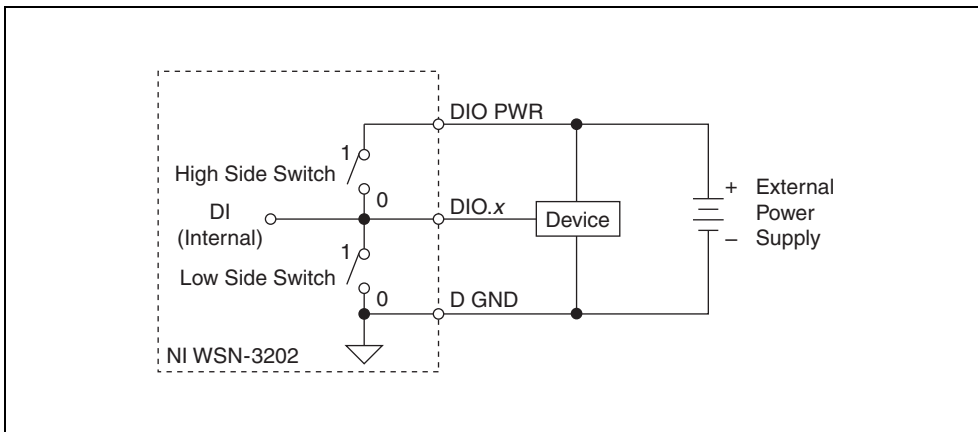


Figure 21. Connecting a Device to the NI WSN-3202 in Drive High and Low Mode

Connecting Sinking Digital Outputs

Drive Low Only Mode

In Drive Low Only mode, the DIO.x terminal is pulled to D GND when you turn on the channel. Writing a digital value of 0 turns on the channel, and 1 turns off the channel. The channel is high impedance when the channel is turned off (1). Use this mode for devices that require low side drive or a sinking output.

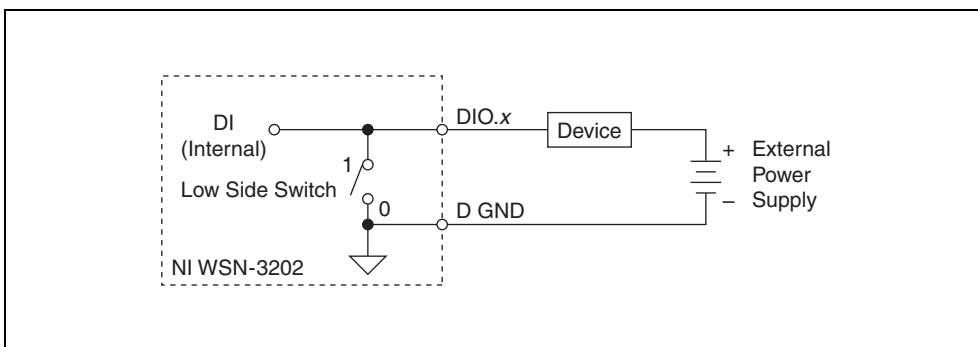


Figure 22. Connecting a Device to the NI WSN-3202 in Drive Low Only Mode

Connecting Digital Inputs

Tristate Mode

Use this mode to configure the channel as digital input, or for contact to ground sensing, as shown in Figure 23. In Tristate mode, when DIO.x terminal is read, a weak pull-up resistor to internal 3.3 V is enabled for about 1 ms.

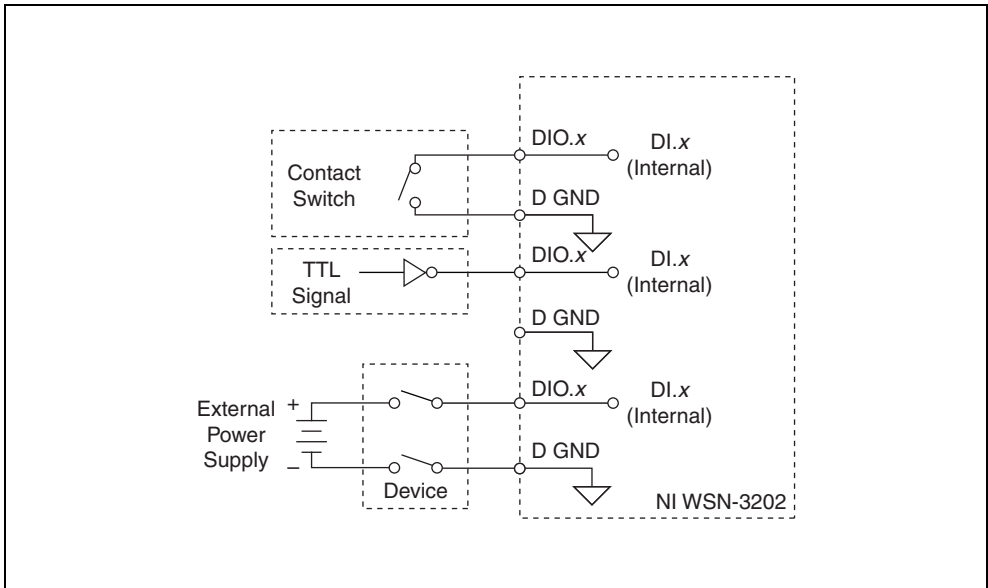


Figure 23. Example of Using the NI WSN-3202 in Tristate Mode

Digital I/O Protection

Each digital I/O channel has overcurrent protection specifically to prevent damage due to short circuit faults.

Understanding Short Circuit Protection

A short circuit fault at the DIO.x terminal may cause a resettable fuse internal to the digital I/O channel to increase in resistance preventing damage to the equipment. Whether the fuse increases in resistance depends on factors such as the current level, the temperature, and power supply voltage. High inrush currents that exist for a short time do not trip the fuse. Refer to the [Specifications](#) section for more information about the maximum continuous output current, short circuit behavior, and short circuit trip time.

Preventing an Overcurrent Condition

Follow these recommendations to prevent an overcurrent condition:

- Do *not* connect DIO PWR to ground.
- Do *not* ground unused terminals.
- Do *not* exceed the output current rating of the channel.

Detecting a Overcurrent Condition

If the node has detected an overcurrent condition, it immediately stops driving the DIO line, goes to a safe power down state, and blinks a four blink error code. The node must be manually reset or power-cycled to resume operation. A DIO line can be in overcurrent if it is driving high, or driving low, but not if it is tristated. To identify which DIO line tripped the overcurrent protection, set all the DIO lines to tristate and one by one set them to the desired drive mode and value until the protection is tripped.

Resetting Channels After an Overcurrent Condition

After you have identified and removed the cause of the overcurrent condition, to resume normal operation, you must reset the node by pressing the RESET button or by removing and reapplying power to the node.

NI WSN-3202 Device Pinout

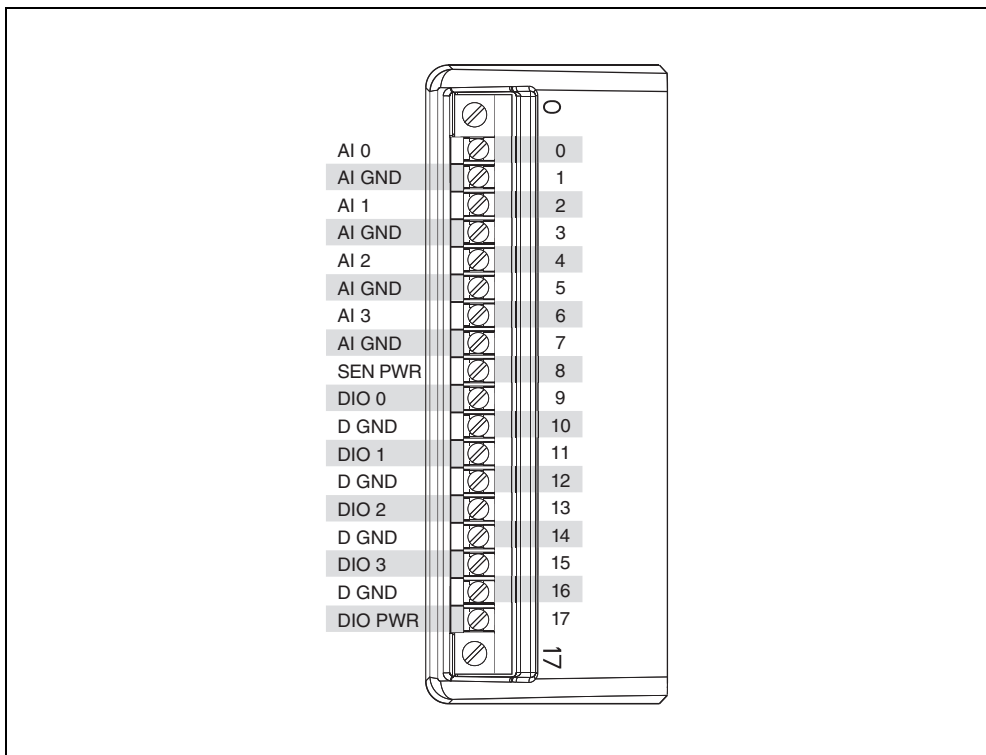


Figure 24. NI WSN-3202 Pinout

Specifications

The following specifications are typical for the range -40 to 70 °C unless otherwise noted.

For the NI WSN gateway specifications, refer to the gateway documentation.

Analog Input Characteristics

Number of channels	4 single-ended
ADC resolution	16 bits
DNL	No missing codes guaranteed
INL	Refer to the Absolute Accuracy Formulas section
Minimum sample interval	1 s
Input coupling	DC
Nominal input ranges	± 10 V, ± 5 V, ± 2 V, ± 0.5 V
Minimum over range	4%
Input impedance (at DC)	
Powered on	>1 G Ω
Powered off/overload	10 k Ω
Input bias current	3 nA
Crosstalk (at 1 kHz)	
Adjacent channels	>100 dB
Non-adjacent channels	>100 dB
Analog bandwidth	7 kHz
Overvoltage protection	± 30 V (one channel only)



Note The values in the following tables are based on calibrated scaling coefficients, which are stored in the onboard EEPROM.

AI Absolute Table Accuracy Summary

Nominal Range (V)	Maximum Absolute Accuracy (mV)* -40 to 70 °C	Typical Absolute Accuracy (mV)* 25 ° ± 5 °C	Random Noise σ (μ Vrms)	Sensitivity [†] (μ V)
± 10	38.21	3.70	342	137
± 5	22.91	2.40	172	68.5
± 2	10.52	1.49	69	27.5
± 0.5	2.69	0.29	18	7
<p>* Absolute accuracy values at full scale on the analog input channels computed using the specified temperature range and are valid for averaging 100 samples immediately following calibration. Refer to the Absolute Accuracy Formulas for more information.</p> <p>[†] Sensitivity is the smallest voltage change that can be detected. It is a function of noise.</p>				

AI Absolute Accuracy Details (Maximum Values)

Nominal Range (V)	Residual Gain Error (ppm of Reading)	Gain Tempco (ppm/°C)	Residual Offset Error (ppm of Range)	Offset Tempco (ppm of Range/°C)	INL Error (ppm of Range)
±10	102	31	164	22	100
±5	137	41	240	22	100
±2	182	48	420	22	100
±0.5	160	50	300	24	100

Absolute Accuracy Formulas

$AbsoluteAccuracy = Reading \cdot GainError + Range \cdot OffsetError + NoiseUncertainty$
 $GainError = ResidualGainError + GainTempco \cdot TempChangeFromLastCal$
 $OffsetError = ResidualOffsetError + OffsetTempco \cdot TempChangeFromLastCal + INL_Error$
 $NoiseUncertainty = (3 \cdot RandomNoise) / \sqrt{NumberOfReadings}$ for a coverage factor of 3 σ and averaging 100 points

Absolute accuracy at full scale on the analog input channels is determined using the following assumptions:

$TempChangeFromLastCal = 45\text{ }^{\circ}\text{C}$
 $NumberOfReadings = 100$
 $CoverageFactor = 3\text{ }\sigma$

For example, on the 10 V range, the absolute accuracy at full scale is as follows:

$GainError = 10\text{ V} \cdot (102\text{ ppm} + 31\text{ ppm} \cdot 45) = 14.97\text{ mV}$
 $OffsetError = 10\text{ V} \cdot (164\text{ ppm} + 22\text{ ppm} \cdot 45 + 100\text{ ppm}) = 12.54\text{ mV}$
 $NoiseUncertainty = 3 \cdot 342\text{ }\mu\text{V}/100^{0.5} = 0.103\text{ mV}$
 $AbsoluteAccuracy = 27.61\text{ mV}$

Sensor Power

Voltage
Typical (10 mA).....12.6 V
Minimum11.5 V
Maximum.....13.35 V

Output Current17 mA maximum at -40 to 70 °C,
20 mA maximum at 25 °C

Delay from sensor power active
to measurement0 ms, 25 ms, 100 ms, 200 ms,
always ON

Digital I/O

Number of channels	4
Modes (per channel)	Bi-directional
Modes (configurable per channel)	Drive High Only, Drive Low Only, Drive High and Low, and Tristate
Power-on output state.....	High Impedance, Tristate
DIO power supply voltage range (V_{DIO_PWR})	5 to 30 V

Digital Input (Tristate Mode)

Input voltage range	0 to 30 V
Digital input logic levels	
High level input voltage	1.7 to 30 V
Low level input voltage.....	0 to 0.45 V
Input current (0 to 30 V)	–160 μ A to 400 μ A, maximum
Contact to ground detection	
Contact close resistance (to ground).....	<2.5 K Ω
Contact open resistance (to ground)	>40 K Ω
Contact capacitance	<20 nF

Digital Output

Total DIO current (all channels)	1 A maximum
Output current (one channel)	0.5 A maximum
Output voltage	
Sourcing	$V_{DIO_PWR} - 0.5\text{ V} - (0.9\ \Omega \times I_{OUT})$ minimum
Sinking	$0.9\ \Omega \times I_{OUT}$ maximum
Protection	
Voltage	30 VDC maximum
Reversed voltage	30 VDC maximum
Short circuit	
Trip current	0.57 A minimum 3.5 A maximum
Trip time.....	2.5 s at 5 A typical at 25 °C
Switching time	
Sinking, 10 K Ω pull-up	15 μ s
Sourcing, 10 K Ω pull-down.....	3.5 ms

Node Resources for LabVIEW WSN

User flash size	248 Kbytes
Number of flash erase cycles per sector	100,000

Wireless Characteristics

Radio mode	IEEE 802.15.4
RF data rate	250 kbit/s
Frequency band ¹	ISM 2.4 GHz (2400 MHz to 2483.5 MHz)
Channels ²	11–24
TX power	
Americas	+17 db (50 mW)
International	+10 db (10 mW)
Range	
Americas	Up to 300 m
International	Up to 150 m
Modulation type	DSSS (O-QPSK)
Receiver sensitivity	–102 dBm
Antenna	
Connector	Female RP-SMA connector
VSWR	MAX 2.0
Impedance	50 Ω
Directivity	Omni
Nominal gain	1.5 dBi

Power Requirements

The following power specifications are typical at 25 °C.

Battery Power



Caution Do *not* use rechargeable batteries.

Internal battery	4 AA 1.5 V alkaline only
Recommended batteries	Energizer EN 91 AA, alkaline Duracell MN1500 AA, alkaline
Battery operating temperature range	
Energizer E91	–18 °C to 55 °C
Duracell MN1500	–20 °C to 54 °C
Voltage range	3.6–7.5 V
Power consumption ³	
60 second sample interval	0.5 mW at 6 V
1 second sample interval	13.3 mW at 6 V

¹ Due to regulations, the frequency bands depend upon the country of operation.

² Due to regulations, the valid channels depend upon country of operation.

³ Device executing NI-WSN firmware. End node mode. Sensor power not used.

Battery life¹

60 second sample interval.....Up to 3 years

1 second sample interval.....Up to 1 month

External Power



Caution You *must* use a UL Listed ITE power supply marked LPS with the NI WSN-3226. The power supply must also meet any safety and compliance requirements for the country of use.

External power9 to 30 V

Power input mating connector2-position mini-combicon,
Phoenix Contact part number: 1714977

Power consumption

End node mode

60 second sample interval.....16 mW at 24 V

1 second sample interval.....33 mW at 24 V

Router mode²300 mW at 24 V

Physical Characteristics

Screw-terminal wiring14 to 24 AWG wire

Torque for screw terminals0.2 to 0.25 N · m

DimensionsRefer to Figure 3 for device dimensions

WeightApproximately 242 g (8.5 oz)

Weight with antennaApproximately 256 g (9 oz)

Calibration

You can obtain the calibration certification and information about calibration services for the NI WSN-3202 at ni.com/calibration. The *NI WSN-3202 Calibration Procedure* is available at ni.com/manuals.

Calibration interval1 year

Safety Standards



Note For UL and other safety certifications, refer to the product label, or go to ni.com/certification, search by model number or product line, and click the appropriate link in the Certification column.

The NI WSN-3202 is designed to meet the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1

¹ Device executing NI-WSN firmware. End node mode. Sensor power not used.

² Router connected directly to gateway. Routing messages for one end node at a one minute sample interval.

Hazardous Locations

U.S. (UL)	Class I, Division 2, Groups A, B, C, D, T4; Class I, Zone 2, AEx nC IIC T4
Canada (C-UL)	Class I, Division 2, Groups A, B, C, D, T4; Class I, Zone 2, Ex nL IIC T4
Europe (DEMKO).....	Ex nA nL IIC T4

Safety Voltages

Connect only voltages that are within these limits.

V terminal to C terminal30 V max, Measurement Category I

Measurement Category I is for measurements performed on circuits not directly connected to the electrical distribution system referred to as MAINS voltage. MAINS is a hazardous live electrical supply system that powers equipment. This category is for measurements of voltages from specially protected secondary circuits. Such voltage measurements include signal levels, special equipment, limited-energy parts of equipment, circuits powered by regulated low-voltage sources, and electronics.



Caution Do *not* connect the system to signals or use for measurements within Measurement Categories II, III, or IV.

RF Safety Warning

This product complies with FCC radiation exposure limits set for uncontrolled equipment and meets the FCC radio frequency (RF) Exposure Guidelines in Supplement C to OET65. This product generates and radiates radio frequency energy. To comply with the radio frequency radiation exposure guidelines in an uncontrolled environment, this equipment should be installed and operated with at least 20 cm between the radiator and the person's body (excluding extremities: hands, wrists, feet, and legs).

This product complies with the European Council Recommendation (1995/519/EC) on the limitation of exposure of the general public to electromagnetic fields. Compliance was determined in accordance with the requirements in EN 50371.

Environmental

Operating temperature (IEC-60068-2-1 and IEC-60068-2-2)	-40 to 70 °C
Storage temperature (IEC-60068-2-1 and IEC-60068-2-2)	-40 to 85 °C
Operating humidity (IEC-60068-2-56).....	10 to 90% RH, noncondensing
Storage humidity (IEC-60068-2-56).....	5 to 95% RH, noncondensing
Pollution Degree (IEC 60664)	2, indoor use only
Maximum altitude.....	2,000 m
Indoor use only	

Shock and Vibration

Operating vibration, random (IEC 60068-2-64).....	5 g _{rms} , 10 to 500 Hz
Operating shock (IEC 60068-2-27)	30 g, 11 ms half sine, 50 g, 3 ms half sine, 18 shocks at 6 orientations
Operating vibration, sinusoidal (IEC 60068-2-6)	5 g, 10 to 500 Hz

Electromagnetic Compatibility



Caution Electromagnetic interference can adversely affect the measurement accuracy of this product. The input/output terminals of this product are not protected for electromagnetic interference. As a result, this device may experience reduced measurement accuracy or other temporary performance degradation when connected cables are routed in an environment with radiated or conducted radio frequency electromagnetic interference. To limit radiated emissions and to ensure that this device functions within specifications in its operational electromagnetic environment, take precautions when designing, selecting, and installing measurement probes and cables.

This product is designed to meet the requirements of the following standards of EMC for electrical equipment for measurement, control, and laboratory use:

- EN 61326-2-1 (IEC 61326-2-1): Class A emissions; Basic immunity
- EN 55011 (CISPR 11): Group 1, Class A emissions
- AS/NZS CISPR 11: Group 1, Class A emissions
- FCC 47 CFR Part 15B: Class A emissions
- ICES-001: Class A emissions

This product also meets the requirements of the following EMC standards for intentional radiators:

- EN 300 328
- EN 301 489-1 and EN 301 489-17
- FCC 47 CFR Part 15C
- IC RSS-210



Note For EMC certification and additional information, refer to the product label or the *Online Product Certification* section.

CE Compliance

This product meets the essential requirements of applicable European Directives, as amended for CE marking, as follows:

- 2006/95/EC; Low-Voltage Directive (safety)
- 2004/108/EC; Electromagnetic Compatibility (EMC) Directive
- 1999/5/EC; Radio and Telecommunications Terminal Equipment (R&TTE) Directive

Regulatory Information

United States

This product complies with Part 15 of the FCC Rules. Operation is subject to these two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Canada

This product complies with Industry Canada RSS-210.

Cet appareil est conforme aux norme RSS210 d'Industrie Canada.

Europe—EU Declaration of Conformity

Marking by the above CE symbol on the label indicates compliance with the Essential Requirements of the R&TTE Directive of the European Union (1999/5/EC). This equipment meets the following conformance standards: EN 300 893, EN300 328, EN301 489-17, EN60950.

Europe – Restrictions for Use of 2.4 GHz Frequencies in European Community Countries

België/ Belgique:	<p>For private usage outside buildings across public grounds over less than 300 m no special registration with IBPT/BIPT is required. Registration to IBPT/BIPT is required for private usage outside buildings across public grounds over more than 300 m. For registration and license please contact IBPT/BIPT.</p> <p>Voor privé-gebruik buiten gebouw over publieke grond over afstand kleiner dan 300 m geen registratie bij BIPT/IBPT nodig; voor gebruik over afstand groter dan 300 m is wel registratie bij BIPT/IBPT nodig. Voor registratie of licentie kunt u contact opnemen met BIPT.</p> <p>Dans le cas d'une utilisation privée, à l'extérieur d'un bâtiment, au-dessus d'un espace public, aucun enregistrement n'est nécessaire pour une distance de moins de 300 m. Pour une distance supérieure à 300 m un enregistrement auprès de l'IBPT est requise. Pour les enregistrements et licences, veuillez contacter l'IBPT.</p>
Deutschland:	<p>License required for outdoor installations. Check with reseller for procedure to follow.</p> <p>Anmeldung im Outdoor-Bereich notwendig, aber nicht genehmigungspflichtig. Bitte mit Händler die Vorgehensweise abstimmen.</p>
France:	<p>Restricted frequency band: only channels 1 to 7 (2400 MHz and 2454 MHz respectively) may be used outdoors in France.</p> <p>Bande de fréquence restreinte : seuls les canaux 1–7 (2400 et 2454 MHz respectivement) doivent être utilisés endroits extérieur en France. Vous pouvez contacter l'Autorité de Régulation des Télécommunications (http://www.art-telecom.fr) pour la procédure à suivre.</p>
Italia:	<p>License required for indoor use. Use with outdoor installations not allowed.</p> <p>E' necessaria la concessione ministeriale anche per l'uso interno.</p> <p>Verificare con i rivenditori la procedura da seguire.</p>
Nederland:	<p>License required for outdoor installations. Check with reseller for procedure to follow.</p> <p>Licentie verplicht voor gebruik met buitenantennes. Neem contact op met verkoper voor juiste procedure.</p>

Japan

The certified radio equipment is embedded in this device.



本機器には認証済み無線設備が内蔵されています

Singapore



Taiwan R.O.C.









低功率電波輻射性電機管理辦法


第十二條經型式認證合格之低功率射頻電機，非經許可，公司、商號或使用者均不得擅自變更頻率、加大功率或變更原設計之特性及功能。

第十四條低功率射頻電機之使用不得影響飛航安全及干擾合法通信；經發現有干擾現象時，應立即停用，並改善至無干擾時方得繼續使用。

前項合法通信，指依電信規定作業之無線電信。低功率射頻電機須忍受合法通信或工業、科學及醫療用電波輻射性電機設備之干擾。

EU Regulatory Statements

 Český [Czech]	<i>National Instruments</i> tímto prohlašuje, že tento NI WSN-3202 je ve shodě se základními požadavky a dalšími příslušnými ustanoveními směrnice 1999/5/ES.
 Dansk [Danish]	Undertegnede <i>National Instruments</i> erklærer herved, at følgende udstyr NI WSN-3202 overholder de væsentlige krav og øvrige relevante krav i direktiv 1999/5/EF.
 Deutsch [German]	Hiermit erklärt <i>National Instruments</i> , dass sich das Gerät NI WSN-3202 in Übereinstimmung mit den grundlegenden Anforderungen und den übrigen einschlägigen Bestimmungen der Richtlinie 1999/5/EG befindet.
 Eesti [Estonian]	Käesolevaga kinnitab <i>National Instruments</i> seadme NI WSN-3202 vastavust direktiivi 1999/5/EÜ põhinõuetele ja nimetatud direktiivist tulenevatele teistele asjakohastele sätetele.
 English	Hereby, <i>National Instruments</i> , declares that this NI WSN-3202 is in compliance with the essential requirements and other relevant provisions of Directive 1999/5/EC.
 Español [Spanish]	Por medio de la presente <i>National Instruments</i> declara que el NI WSN-3202 cumple con los requisitos esenciales y cualesquiera otras disposiciones aplicables o exigibles de la Directiva 1999/5/CE.
 Ελληνική [Greek]	ΜΕ ΤΗΝ ΠΑΡΟΥΣΑ <i>National Instruments</i> ΔΗΛΩΝΕΙ ΟΤΙ ΝΙ WSN-3202 ΣΥΜΜΟΡΦΩΝΕΤΑΙ ΠΡΟΣ ΤΙΣ ΟΥΣΙΩΔΕΙΣ ΑΠΑΙΤΗΣΕΙΣ ΚΑΙ ΤΙΣ ΛΟΙΠΕΣ ΣΧΕΤΙΚΕΣ ΔΙΑΤΑΞΕΙΣ ΤΗΣ ΟΔΗΓΙΑΣ 1999/5/ΕΚ.
 Français [French]	Par la présente <i>National Instruments</i> déclare que l'appareil NI WSN-3202 est conforme aux exigences essentielles et aux autres dispositions pertinentes de la directive 1999/5/CE.

 Italiano [Italian]	Con la presente <i>National Instruments</i> dichiara che questo NI WSN-3202 è conforme ai requisiti essenziali ed alle altre disposizioni pertinenti stabilite dalla direttiva 1999/5/CE.
 Latviski [Latvian]	Ar šo <i>National Instruments</i> deklarē, ka NI WSN-3202 atbilst Direktīvas 1999/5/EK būtiskajām prasībām un citiem ar to saistītajiem noteikumiem.
 momLietuvių [Lithuanian]	Šiuo <i>National Instruments</i> deklaruoją, kad šis NI WSN-3202 atitinka esminius reikalavimus ir kitas 1999/5/EB Direktyvos nuostatas.
 Nederlands [Dutch]	Hierbij verklaart <i>National Instruments</i> dat het toestel NI WSN-3202 in overeenstemming is met de essentiële eisen en de andere relevante bepalingen van richtlijn 1999/5/EG.
 Malti [Maltese]	Hawnhekk, <i>National Instruments</i> , jiddikjara li dan NI WSN-3202 jikkonforma mal-htigijiet essenzjali u ma provvedimenti oħrajn rilevanti li hemm fid-Direttiva 1999/5/EC.
 Magyar [Hungarian]	Alulírott, <i>National Instruments</i> nyilatkozom, hogy a NI WSN-3202 megfelel a vonatkozó alapvető követelményeknek és az 1999/5/EC irányelv egyéb előírásainak.
 Polski [Polish]	Niniejszym <i>National Instruments</i> . oświadcza, że NI WSN-3202 jest zgodny z zasadniczymi wymogami oraz pozostałymi stosownymi postanowieniami Dyrektywy 1999/5/EC.
 Português [Portuguese]	<i>National Instruments</i> declara que este NI WSN-3202 está conforme com os requisitos essenciais e outras disposições da Directiva 1999/5/CE.
 Slovensko [Slovenian]	<i>National Instruments</i> izjavlja, da je ta NI WSN-3202 v skladu z bistvenimi zahtevami in ostalimi relevantnimi določili direktive 1999/5/ES.
 Slovensky [Slovak]	<i>National Instruments</i> týmto vyhlasuje, že NI WSN-3202 spĺňa základné požiadavky a všetky príslušné ustanovenia Smernice 1999/5/ES.
 Suomi [Finnish]	<i>National Instruments</i> vakuuttaa täten että NI WSN-3202 tyyppinen laite on direktiivin 1999/5/EY oleellisten vaatimusten ja sitä koskevien direktiivin muiden ehtojen mukainen.
 Svenska [Swedish]	Härmed intygar <i>National Instruments</i> att denna NI WSN-3202 står i överensstämmelse med de väsentliga egenskapskrav och övriga relevanta bestämmelser som framgår av direktiv 1999/5/EG.
Íslenska [Icelandic]	Hér með lýsir <i>National Instruments</i> yfir því að NI WSN-3202 er í samræmi við grunnkröfur og aðrar kröfur, sem gerðar eru í tilskipun 1999/5/EC.
 Norsk [Norwegian]	<i>National Instruments</i> erklærer herved at utstyret NI WSN-3202 er i samsvar med de grunnleggende krav og øvrige relevante krav i direktiv 1999/5/EF.

Online Product Certification

Refer to the product Declaration of Conformity (DoC) for additional regulatory compliance information. To obtain product certifications and the DoC for this product, visit ni.com/certification, search by model number or product line, and click the appropriate link in the certification column.

Environmental Management

NI is committed to designing and manufacturing products in an environmentally responsible manner. NI recognizes that eliminating certain hazardous substances from our products is beneficial to the environment and to NI customers.

For additional environmental information, refer to the *NI and the Environment* Web page at ni.com/environment. This page contains the environmental regulations and directives with which NI complies, as well as other environmental information not included in this document.

Waste Electrical and Electronic Equipment (WEEE)



EU Customers At the end of the product life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers, National Instruments WEEE initiatives, and compliance with WEEE Directive 2002/96/EC on Waste and Electronic Equipment, visit ni.com/environment/wee.

Battery Replacement and Disposal



Battery Directive After replacement, recycle the old battery. For information about the available collection and recycling scheme (and your nearest National Instruments Branch Office) or on Battery Directive compliance (Directive 2006/66/EC of the European Parliament and Council) in a particular EU country visit ni.com/company/citizenship/product.htm#battery.

电子信息产品污染控制管理办法（中国 RoHS）



中国客户 National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于 National Instruments 中国 RoHS 合规性信息, 请登录 ni.com/environment/rohs_china。(For information about China RoHS compliance, go to ni.com/environment/rohs_china.)

Where to Go for Support

The National Instruments Web site is your complete resource for technical support. At ni.com/support you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world to help address your support needs. For telephone support in the United States, create your service request at ni.com/support and follow the calling instructions or dial 512 795 8248. For telephone support outside the United States, contact your local branch office:

Australia 1800 300 800, Austria 43 662 457990-0, Belgium 32 (0) 2 757 0020,
Brazil 55 11 3262 3599, Canada 800 433 3488, China 86 21 5050 9800,
Czech Republic 420 224 235 774, Denmark 45 45 76 26 00, Finland 358 (0) 9 725 72511,
France 01 57 66 24 24, Germany 49 89 7413130, India 91 80 41190000, Israel 972 3 6393737,
Italy 39 02 41309277, Japan 0120-527196, Korea 82 02 3451 3400, Lebanon 961 (0) 1 33 28 28,
Malaysia 1800 887710, Mexico 01 800 010 0793, Netherlands 31 (0) 348 433 466,
New Zealand 0800 553 322, Norway 47 (0) 66 90 76 60, Poland 48 22 328 90 10,
Portugal 351 210 311 210, Russia 7 495 783 6851, Singapore 1800 226 5886,
Slovenia 386 3 425 42 00, South Africa 27 0 11 805 8197, Spain 34 91 640 0085,
Sweden 46 (0) 8 587 895 00, Switzerland 41 56 2005151, Taiwan 886 02 2377 2222,
Thailand 662 278 6777, Turkey 90 212 279 3031, United Kingdom 44 (0) 1635 523545

LabVIEW, National Instruments, NI, ni.com, the National Instruments corporate logo, and the Eagle logo are trademarks of National Instruments Corporation. Refer to the *Trademark Information* at ni.com/trademarks for other National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patent Notice* at ni.com/patents.